


LEVEL
25.10.2009
12:30:31

Output: Analog
Imp: 600Ohm
Sine
0.01dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -19.9dBV 249.9 Hz

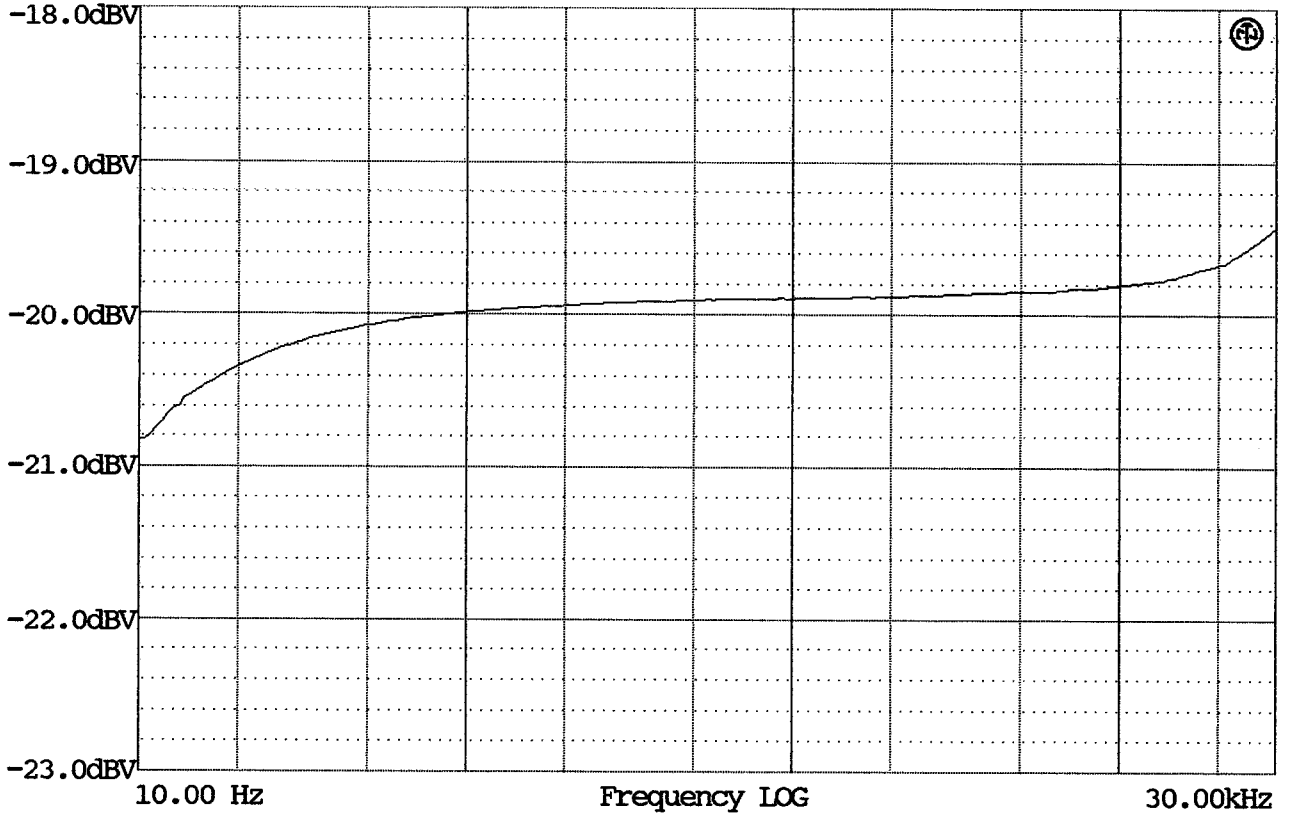


THD+N
25.10.2009
13:32:51

Output: Analog
Imp: 600Ohm
Sine
0.01dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -19.9dBV 249.9 Hz

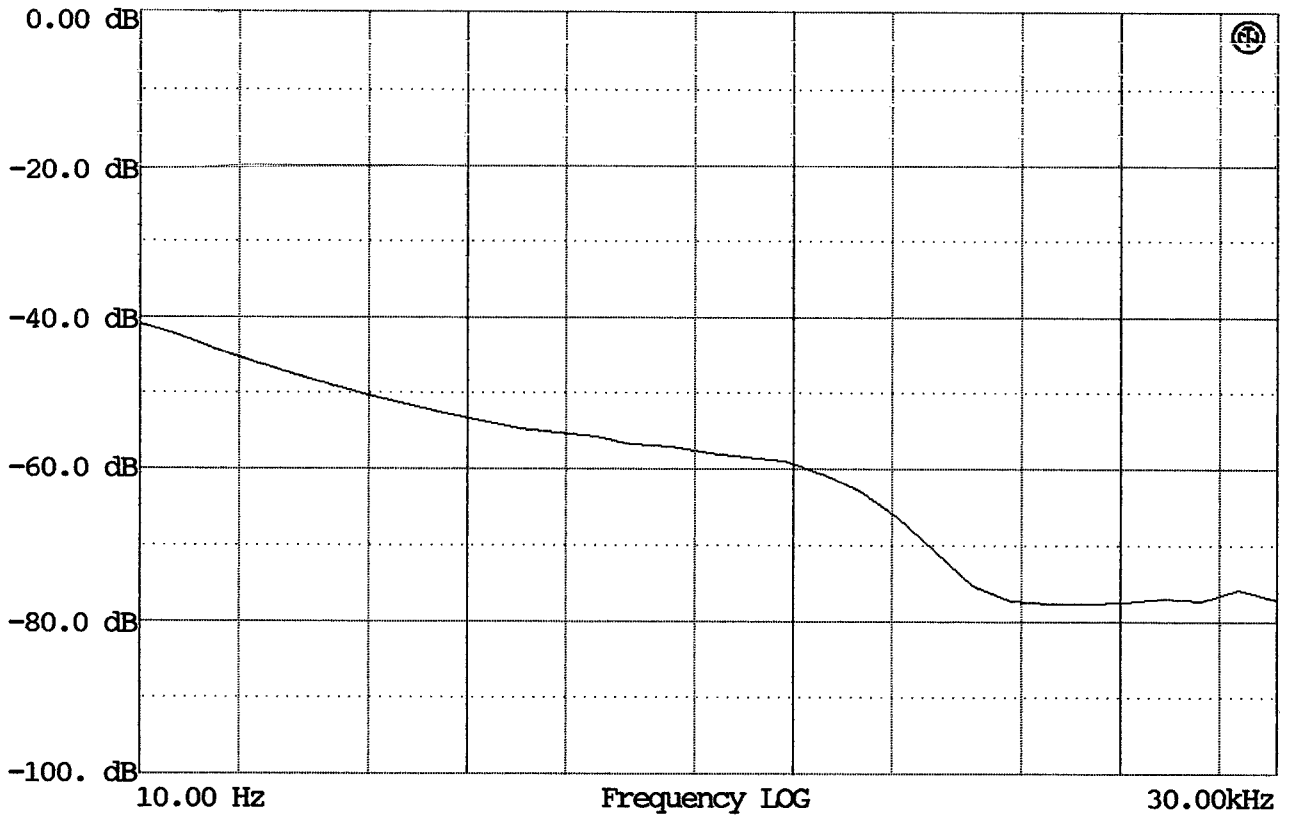

STAGE 4HE dB-100


THD+N
25.10.2009
13:38:18

Output: Analog
Imp: 600Ohm
Sine
10.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -9.88dBV 249.9 Hz

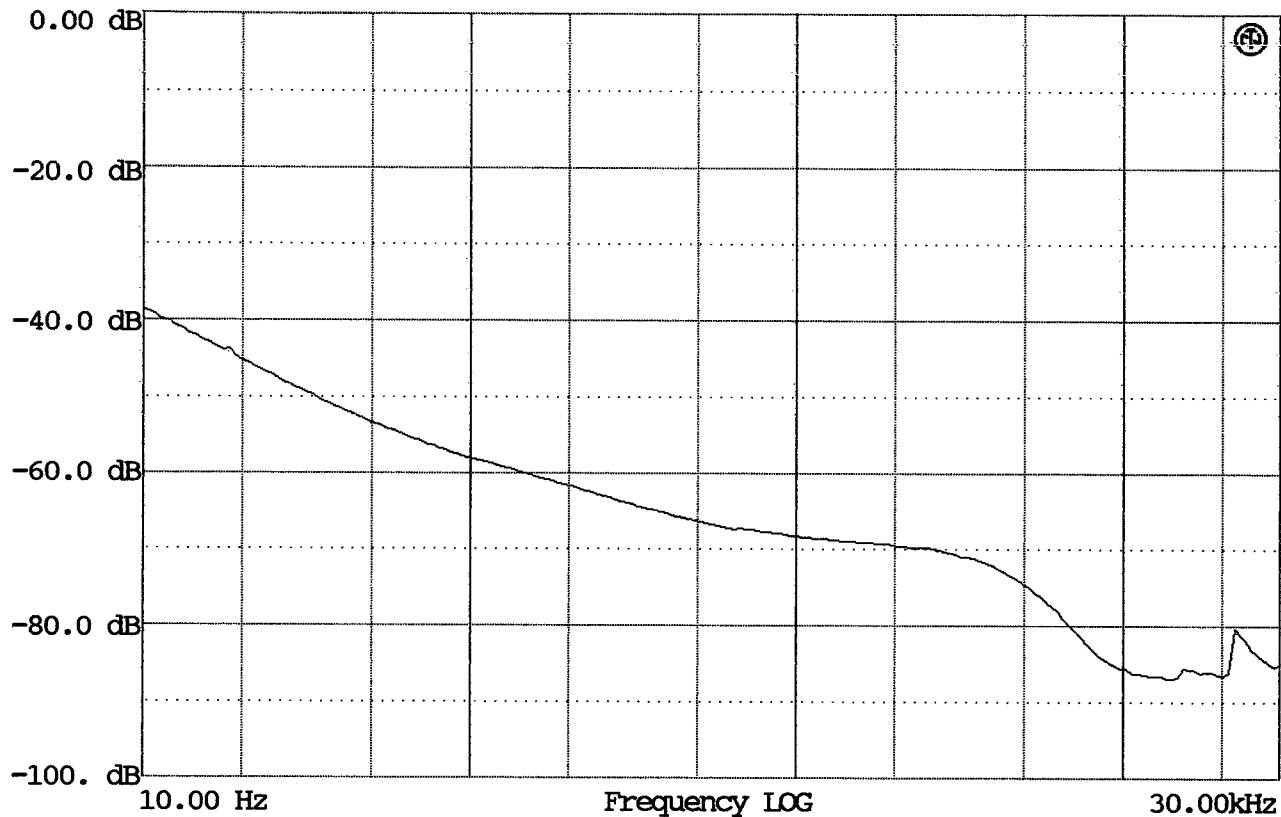


THD+N
25.10.2009
13:44:30

Output: Analog
Imp: 600Ohm
Sine
-10.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
AUDIOBP

A: -30.0dBV 249.9 Hz

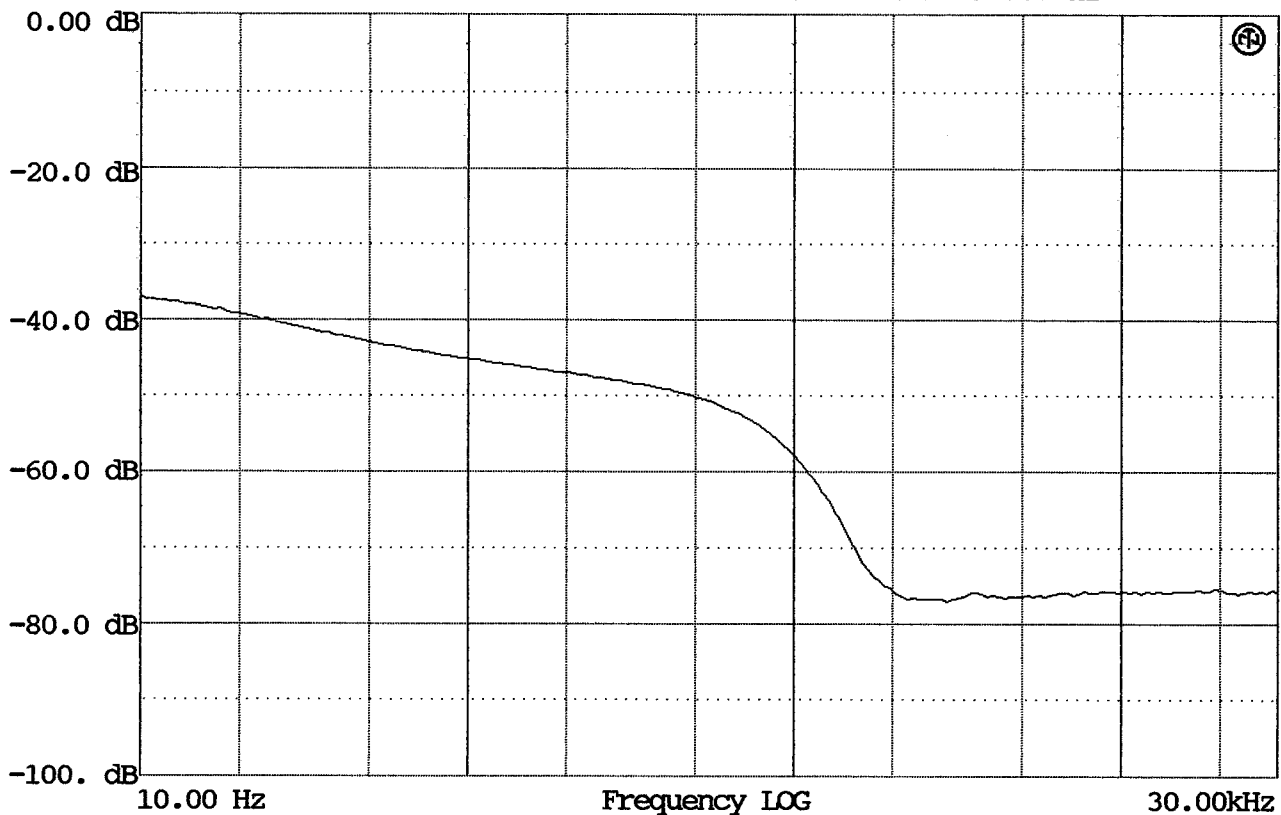

STAGE LINE 01B-600


LEVEL
25.10.2009
13:46:32

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 0.17dBV 249.9 Hz

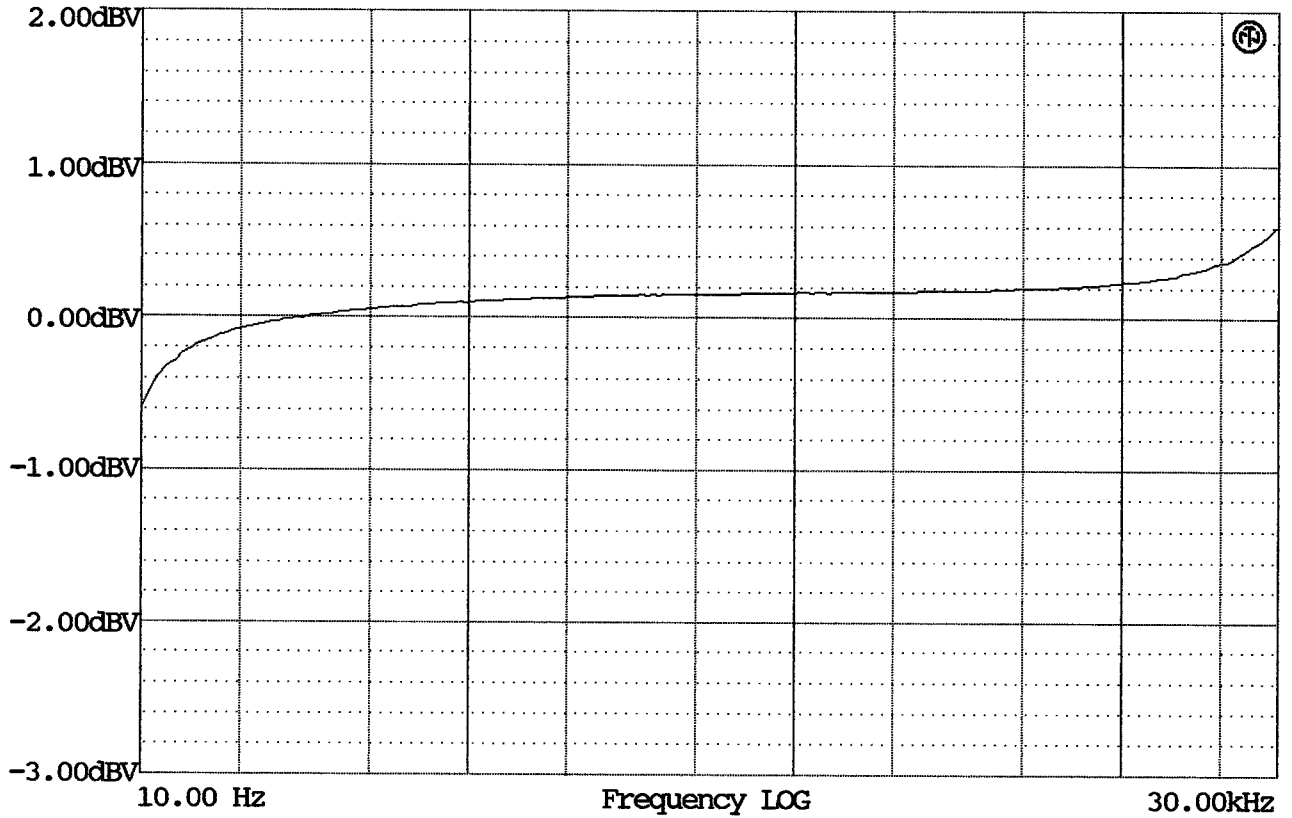


THD+N
25.10.2009
13:54:20

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 0.17dBV 249.9 Hz

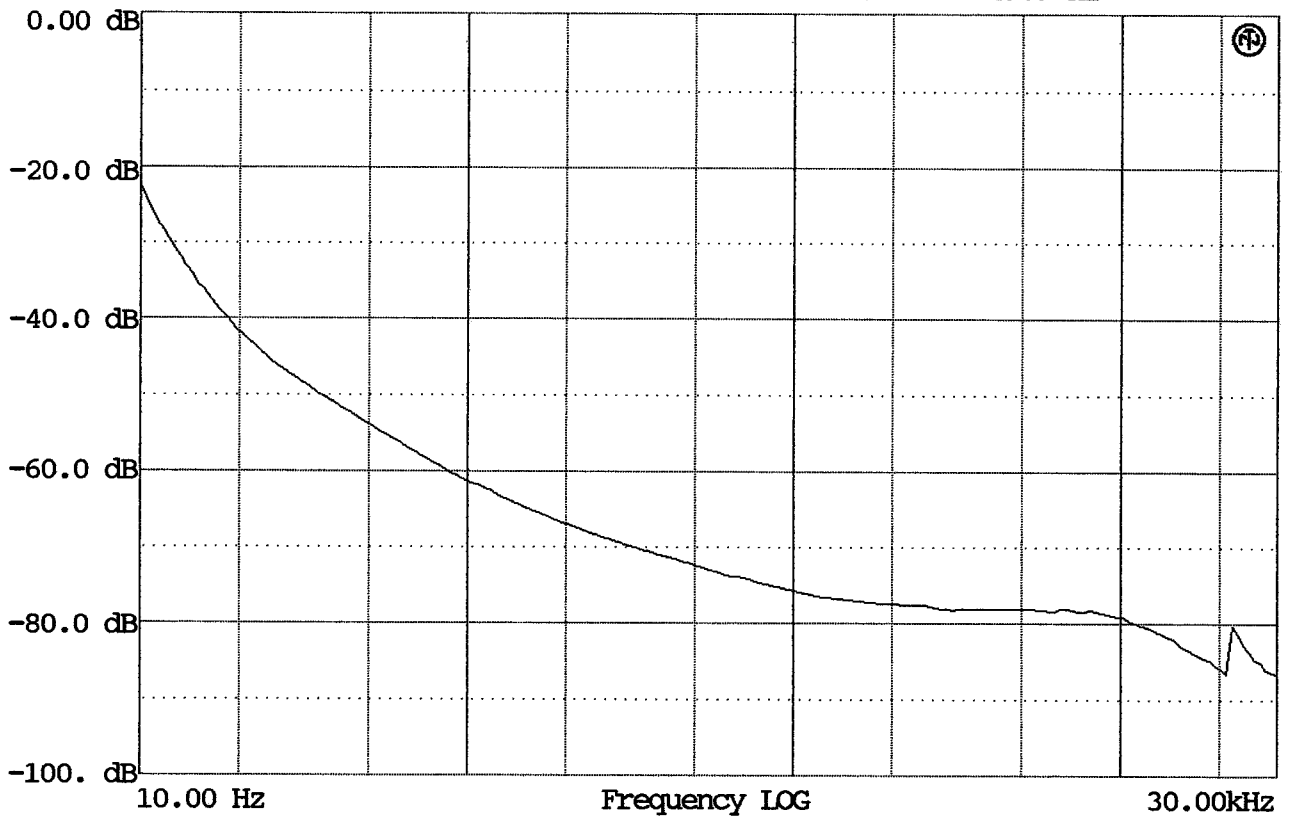

STAGE 4Hz 0dB-100


LEVEL
25.10.2009
13:56:23

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -19.7dBV 249.9 Hz

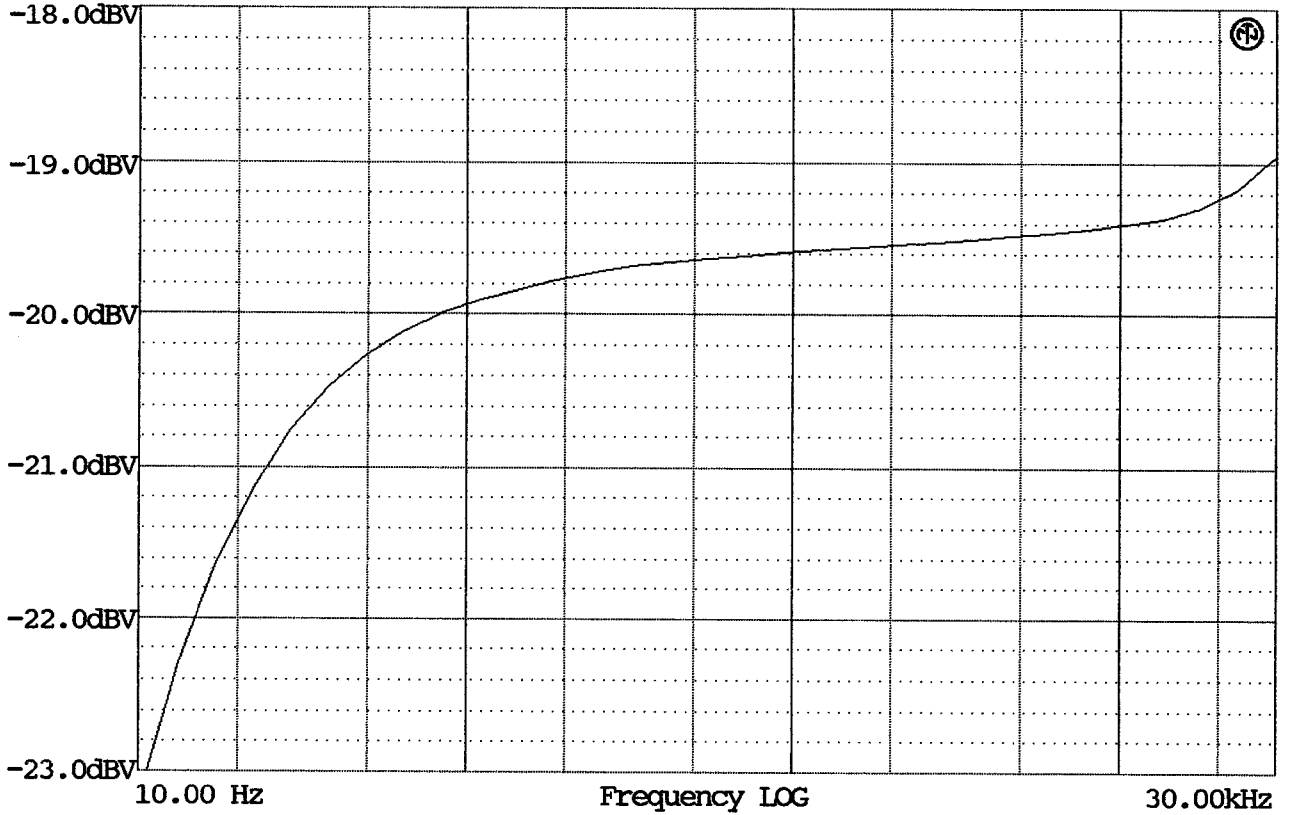


LEVEL
25.10.2009
13:57:29

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -40.2dBV 249.9 Hz

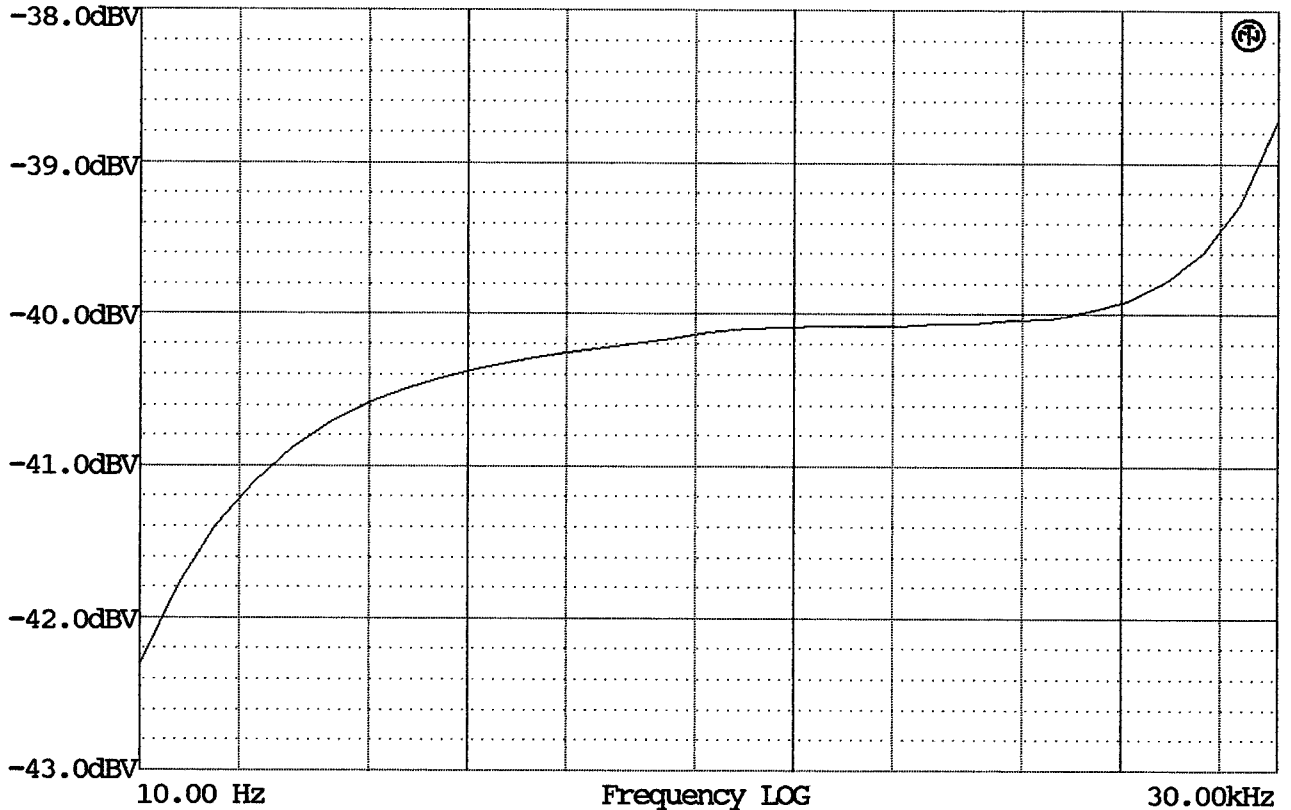


STAGE 41B DIB-100

~~THD+N~~
25.10.2009
14:06:43

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm
A: -19.7dBV 249.9 Hz

Filter:
AUDIOBP

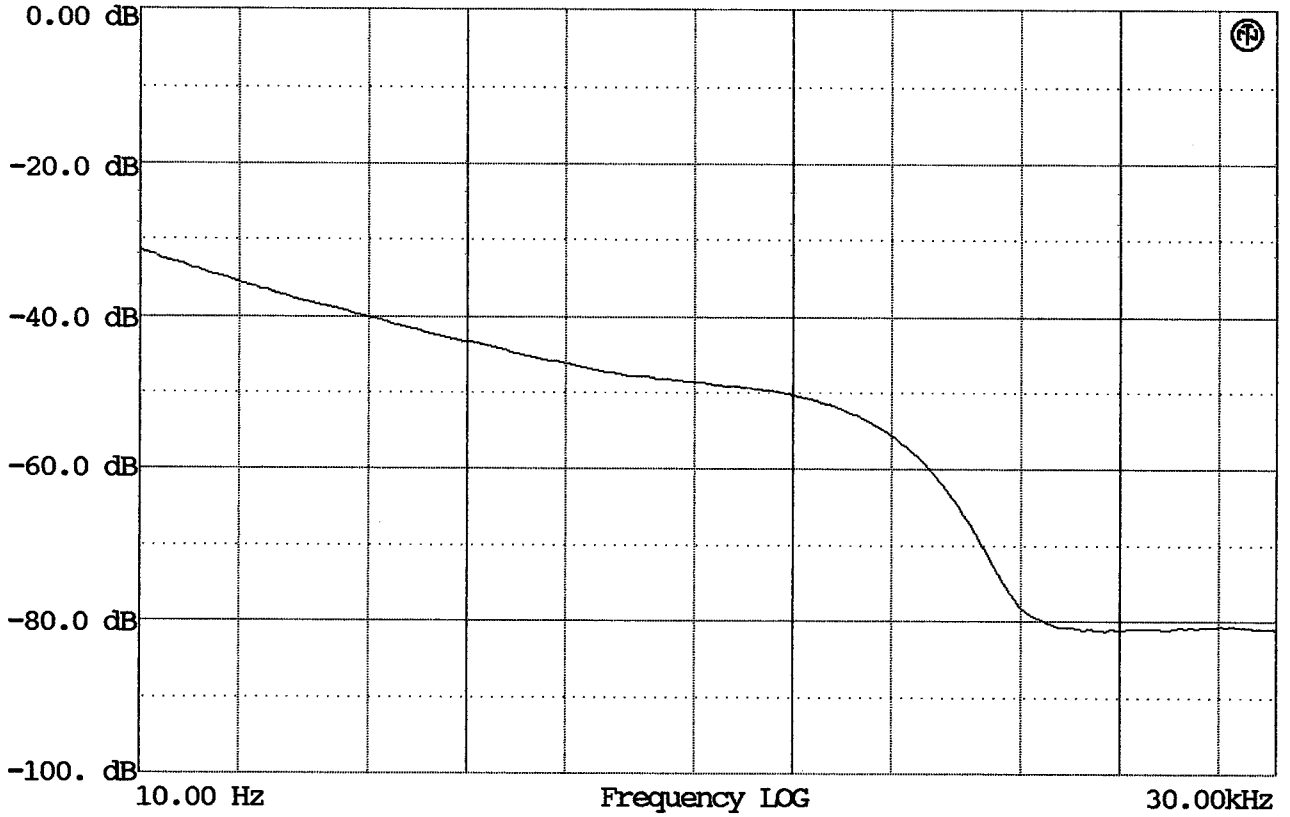


~~THD+N~~
25.10.2009
14:17:39

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 250.0 Hz

Input: Analog
Imp: 100kOhm
A: -40.2dBV 249.9 Hz

Filter:
AUDIOBP

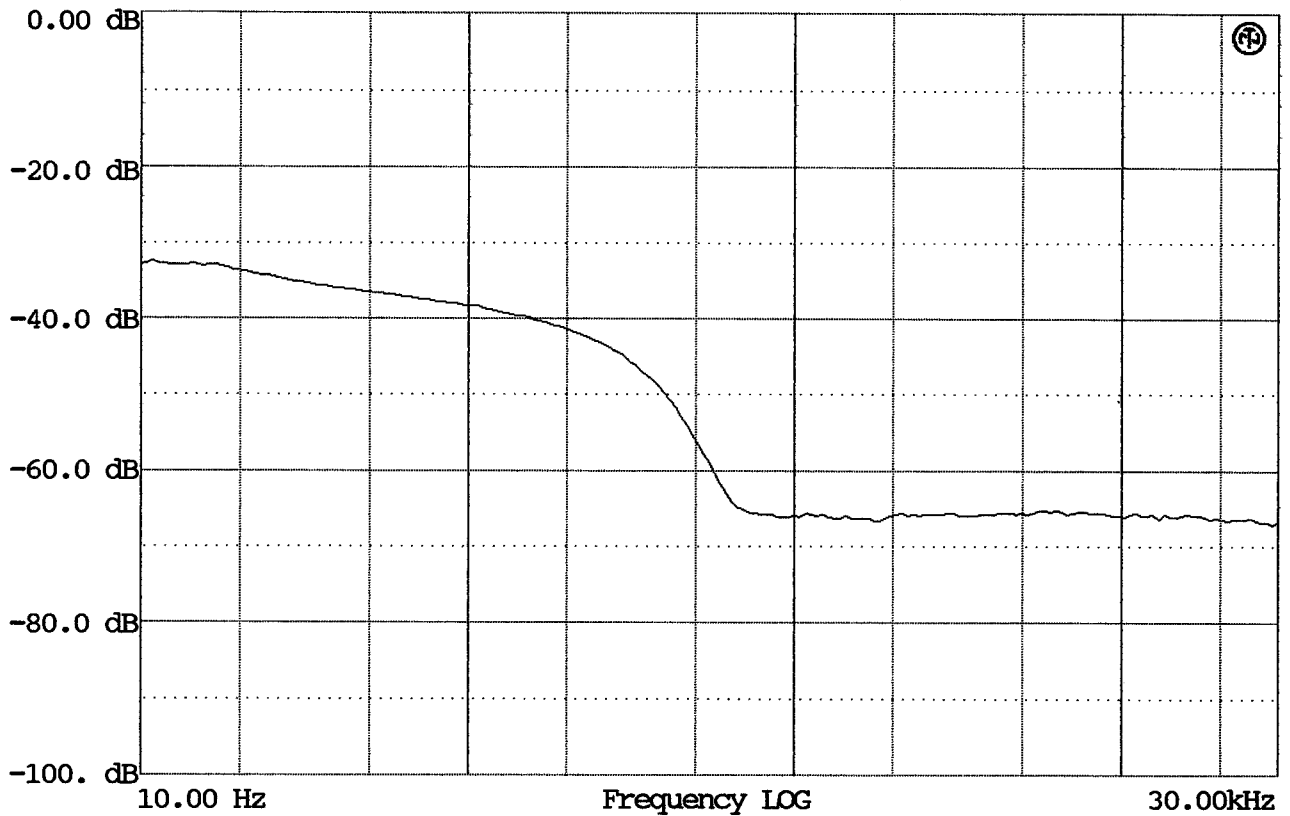

STAGE LINE 018-100