


LEVEL
02.07.2011
13:45:44

Output: Analog
Imp: <150hm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp:100kOhm
A:-14.0dBV 39.99 Hz

Filter:
Off

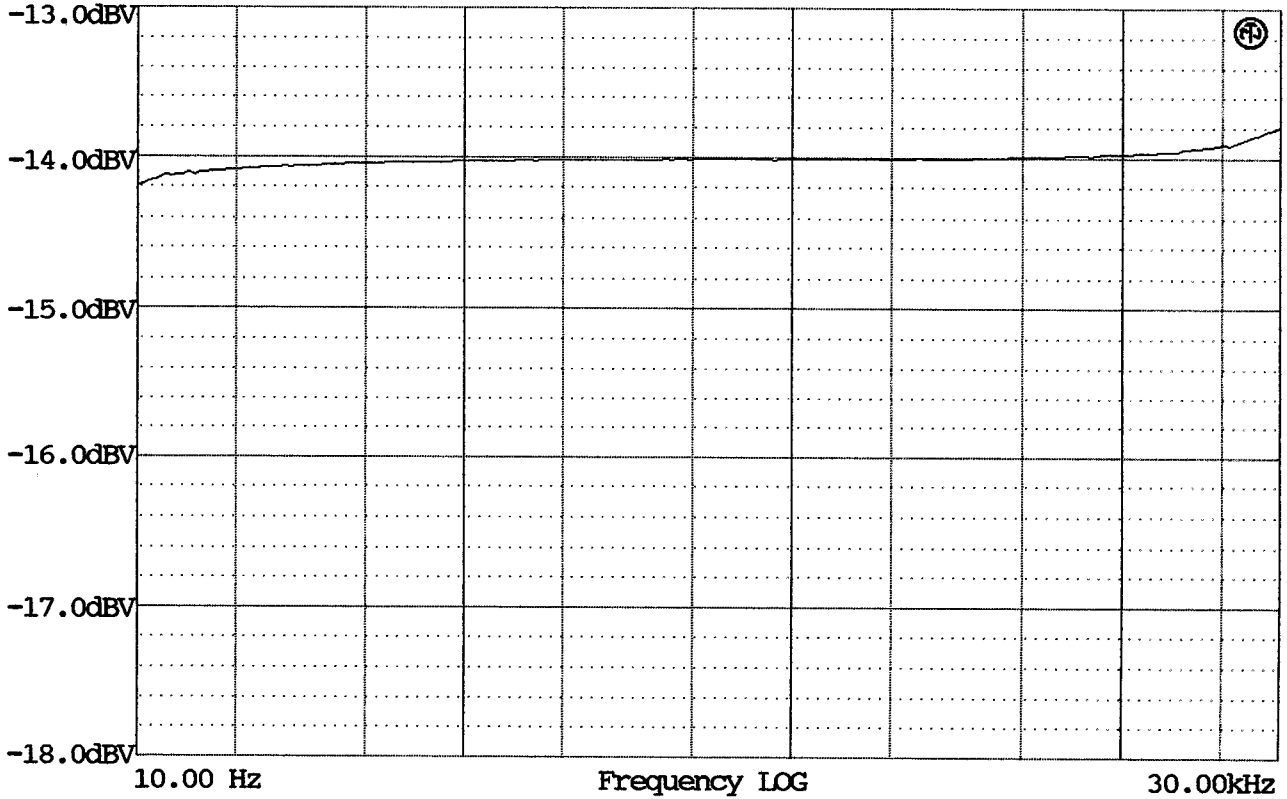


THD+N
02.07.2011
13:51:30

Output: Analog
Imp: <150hm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp:100kOhm
A:-14.0dBV 39.99 Hz

Filter:
AUDIOBP

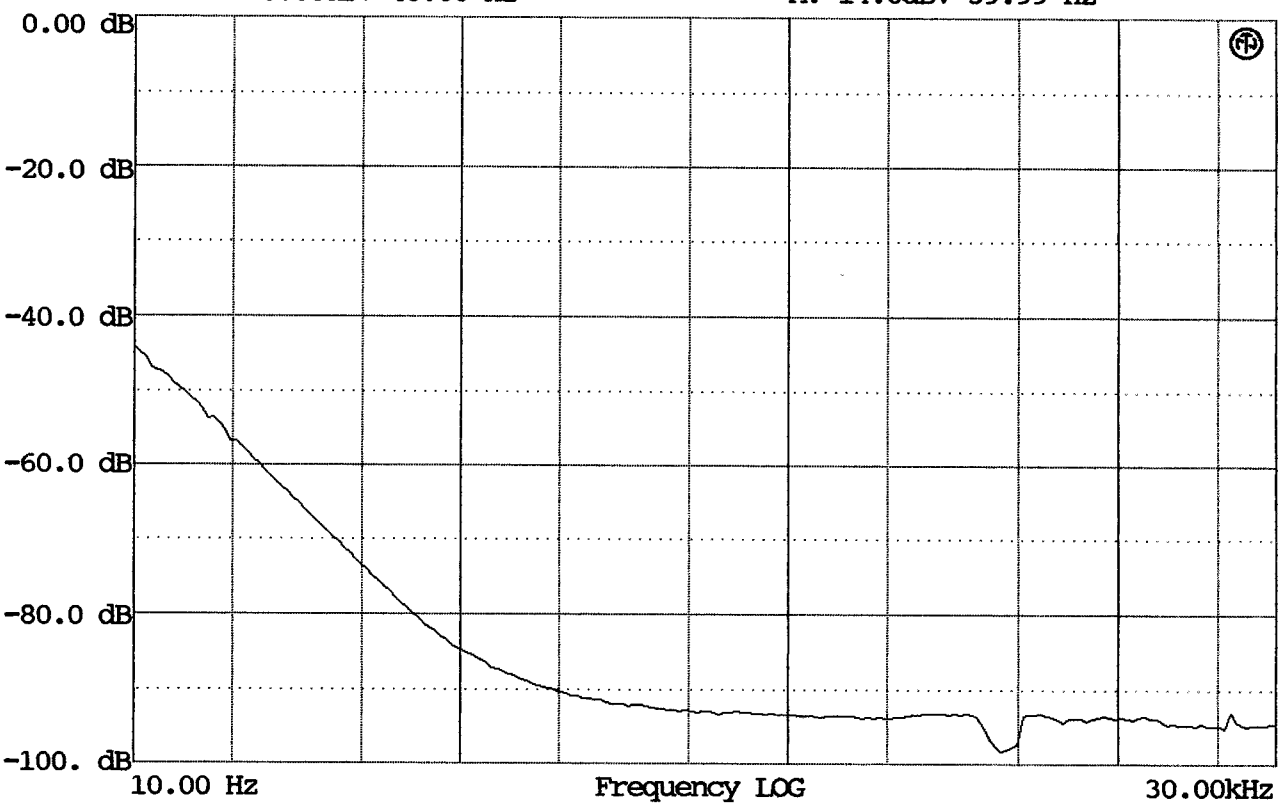

LEVEL
02.07.2011
13:53:08

Output: Analog
Imp: 200Ohm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp: 100kOhm
A: -14.1dBV 39.99 Hz

Filter:
Off




THD+N
02.07.2011
13:58:54

Output: Analog
Imp: 200Ohm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp: 100kOhm
A: -14.1dBV 39.99 Hz

Filter:
AUDIOBP

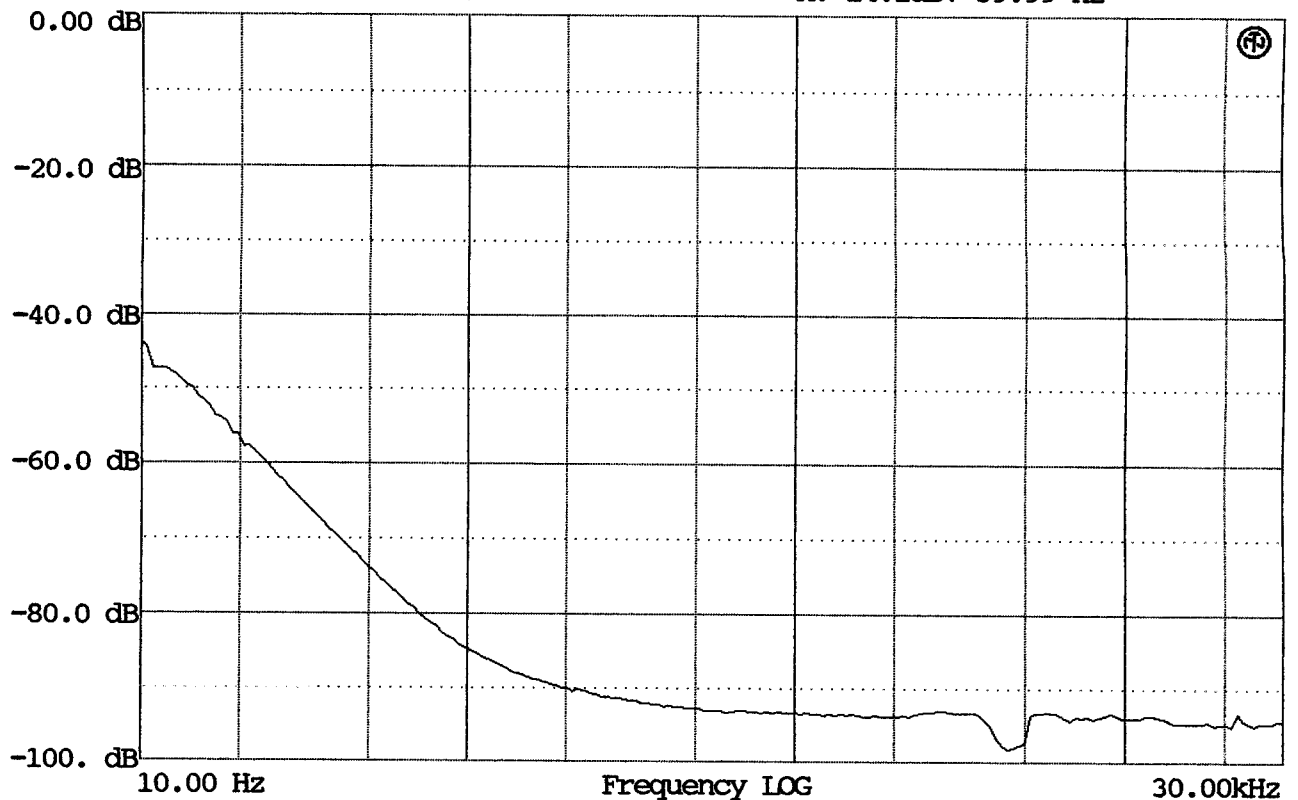


LEVEL
02.07.2011
14:00:33

Output: Analog
Imp: 600Ohm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -14.3dBV 39.99 Hz

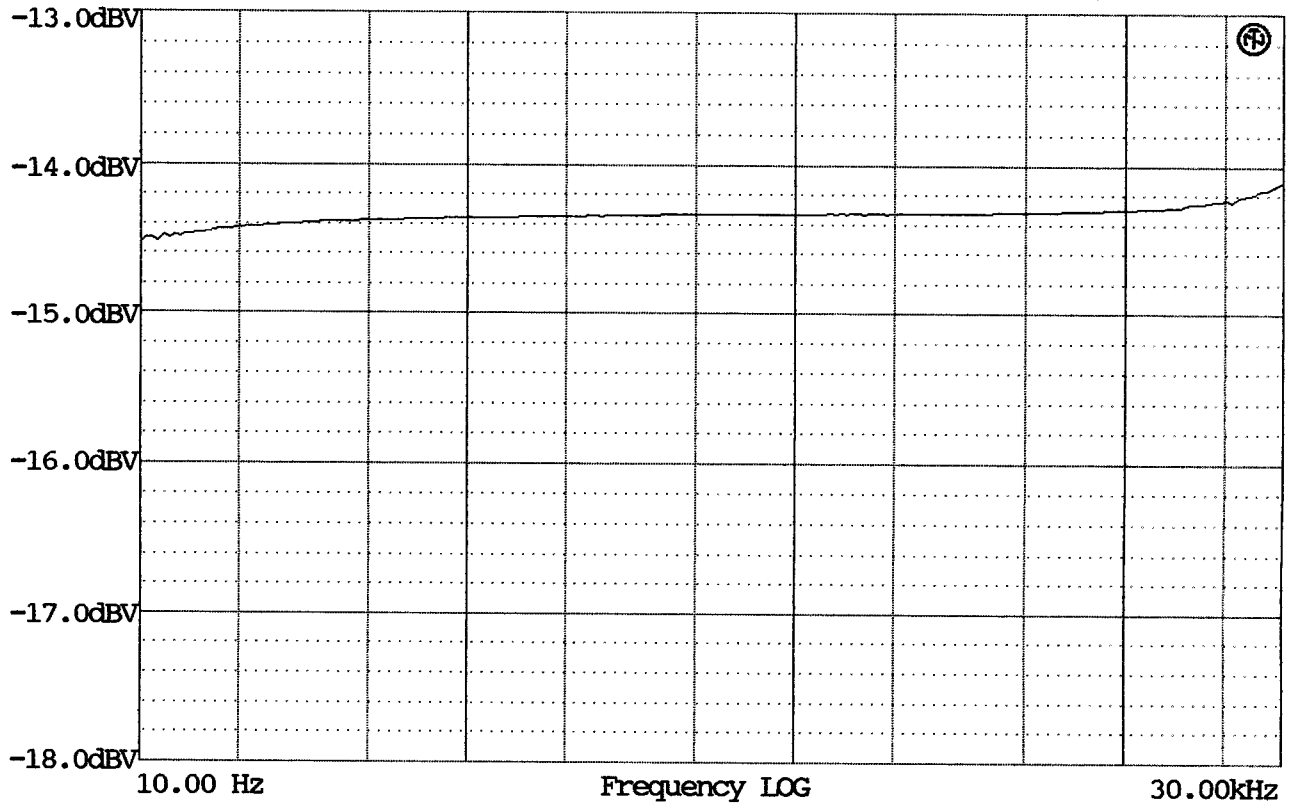


THD+N
02.07.2011
14:06:23

Output: Analog
Imp: 600Ohm
Sine
0.00dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
AUDIOBP

A: -14.3dBV 39.99 Hz

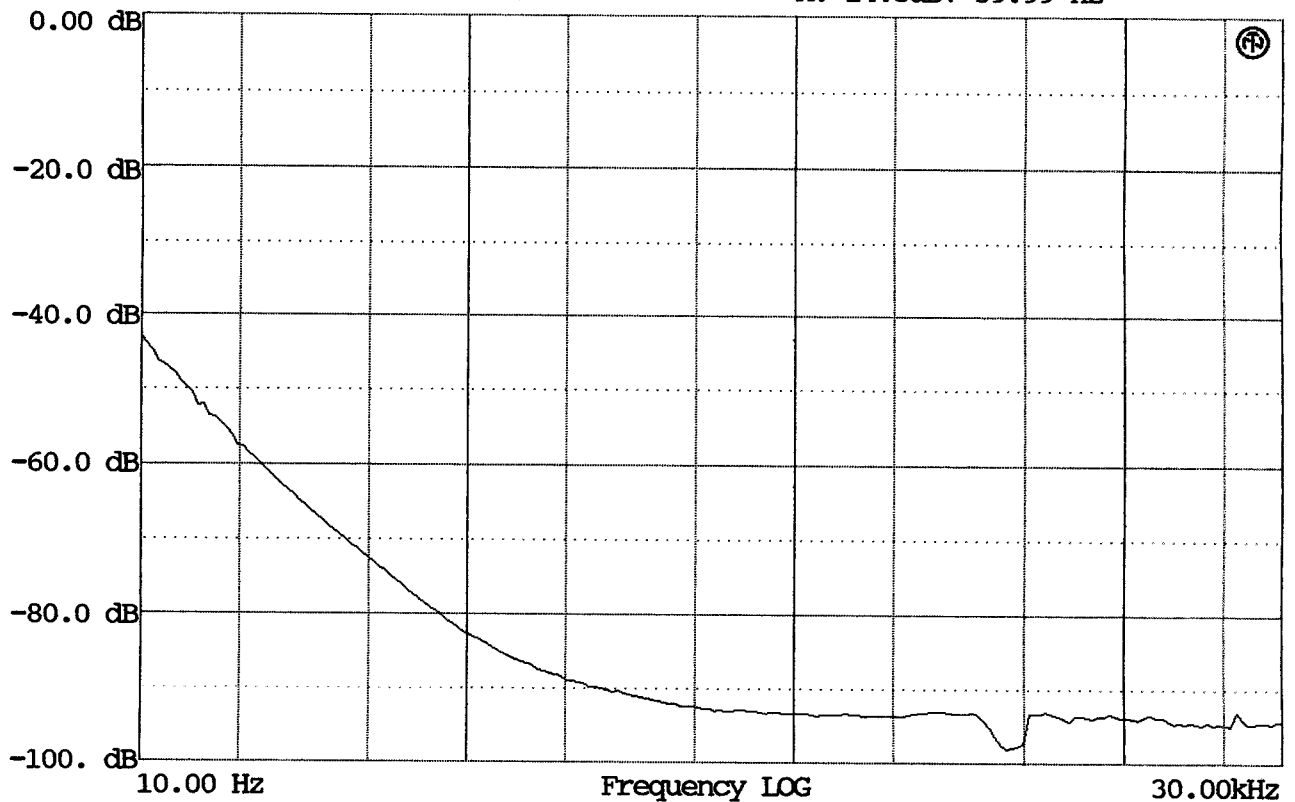


LEVEL
02.07.2011
14:10:26

Output: Analog
Imp: <150hm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp:100kOhm

Filter:
Off

A:-4.03dBV 39.99 Hz

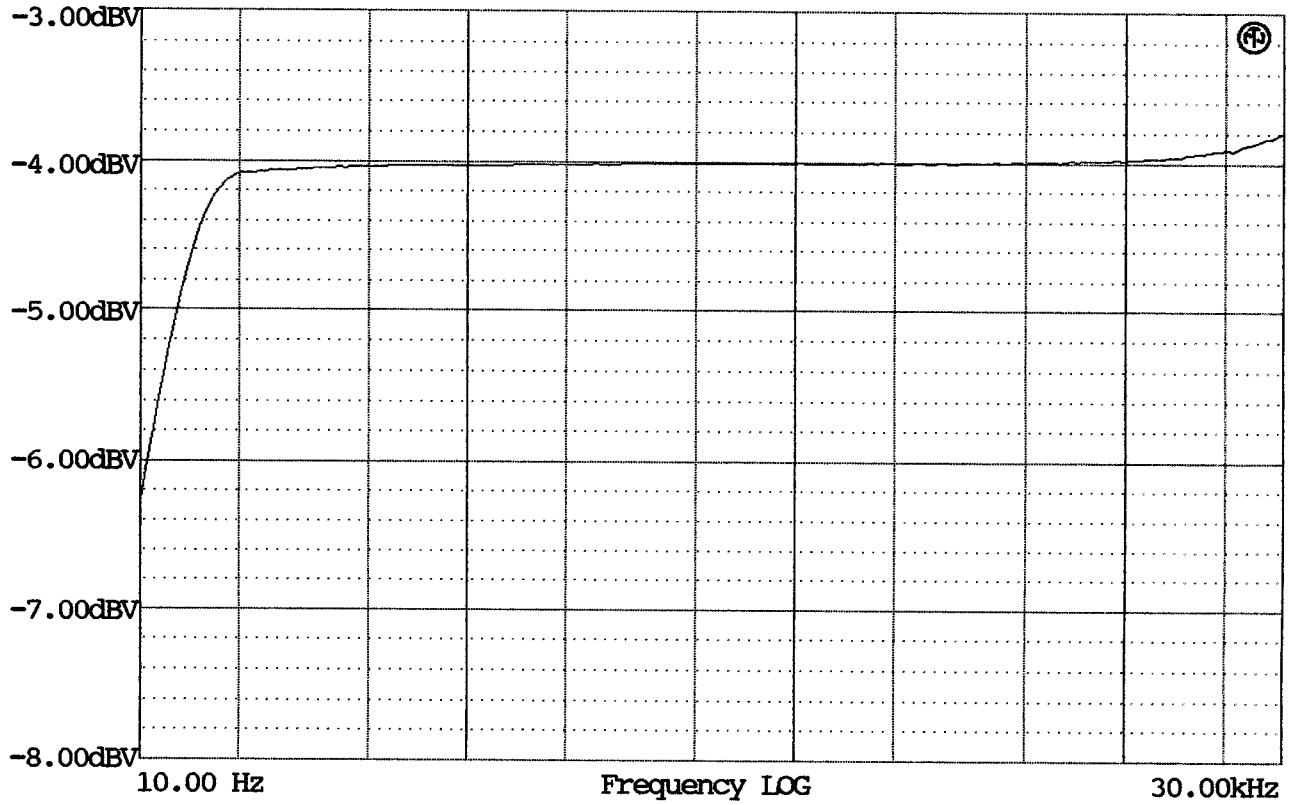


THD+N
02.07.2011
14:32:07

Output: Analog
Imp: <150hm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp:100kOhm

Filter:
Off

A:-4.03dBV 39.99 Hz

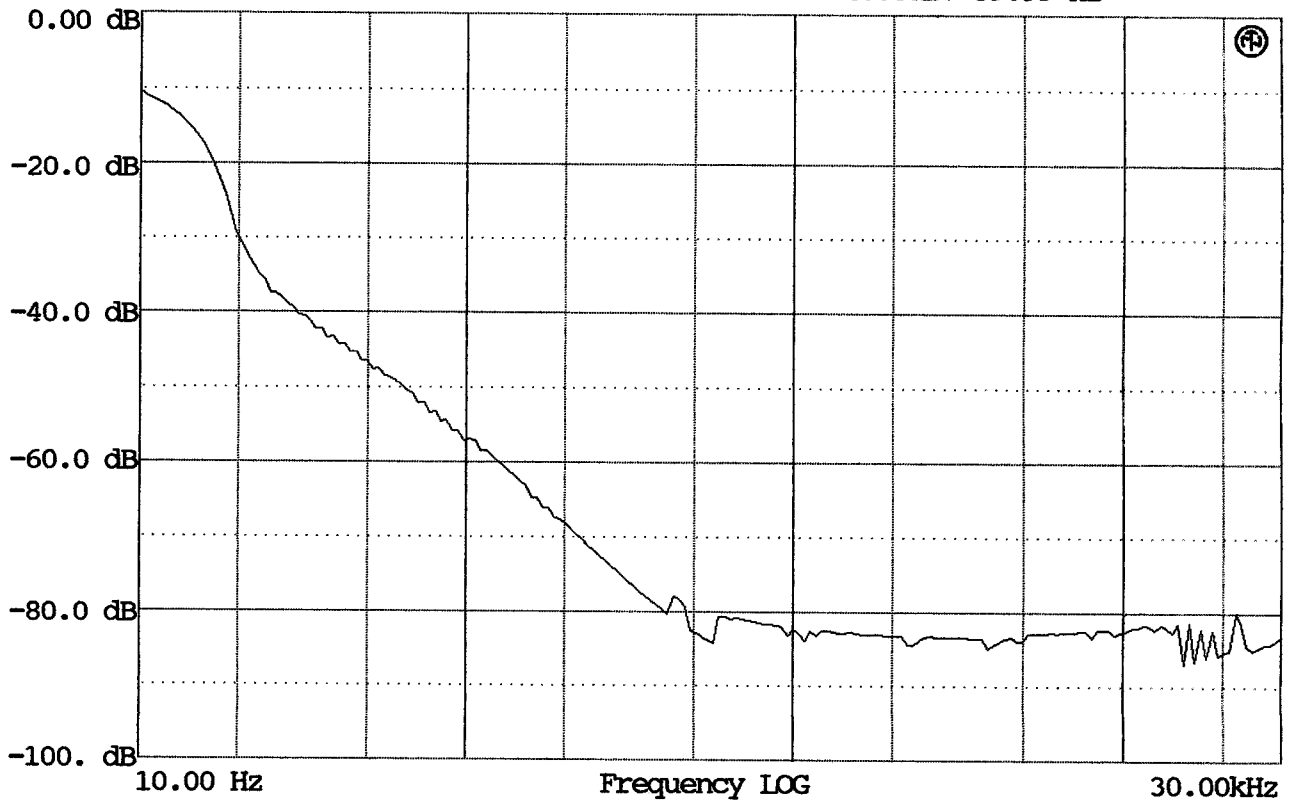


LEVEL
02.07.2011
14:39:03

Output: Analog
Imp: 200Ohm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -4.14dBV 39.99 Hz

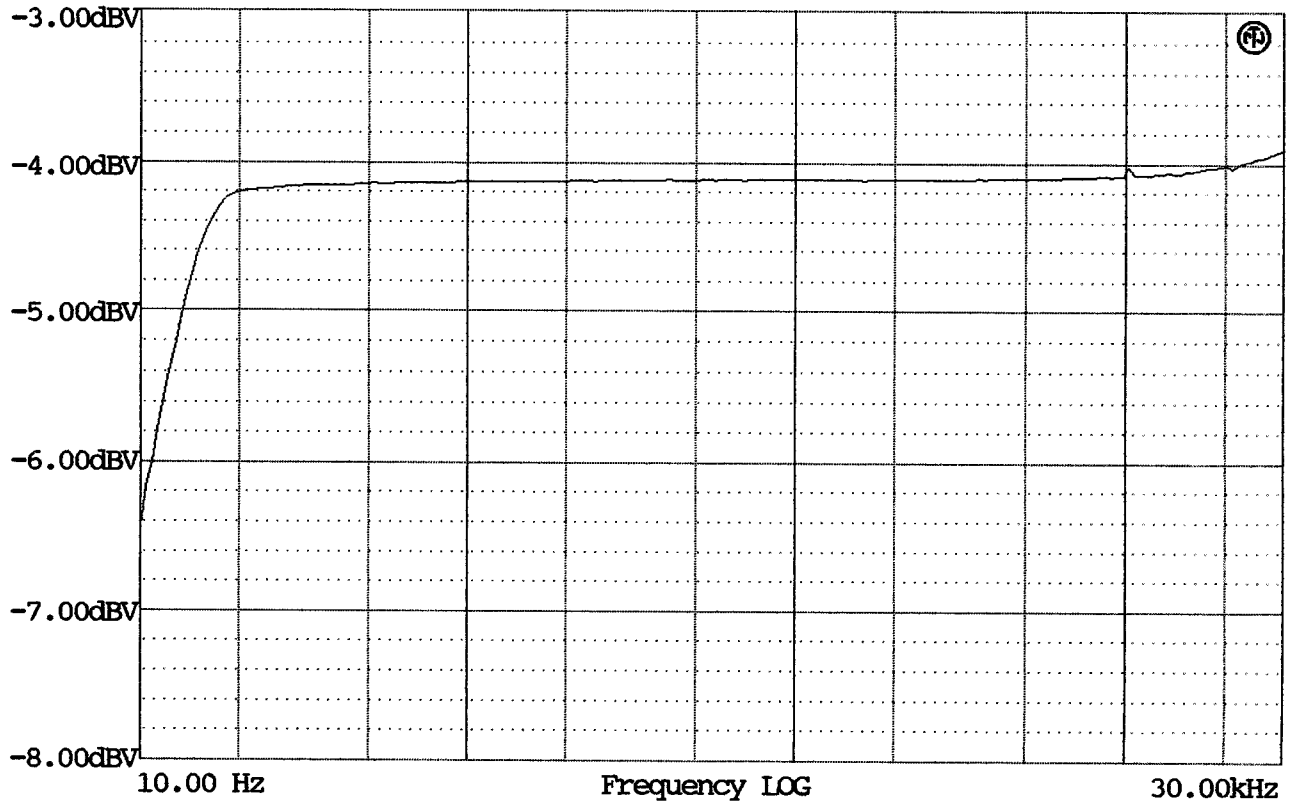


THD+N
02.07.2011
15:00:00

Output: Analog
Imp: 200Ohm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: -4.13dBV 39.99 Hz

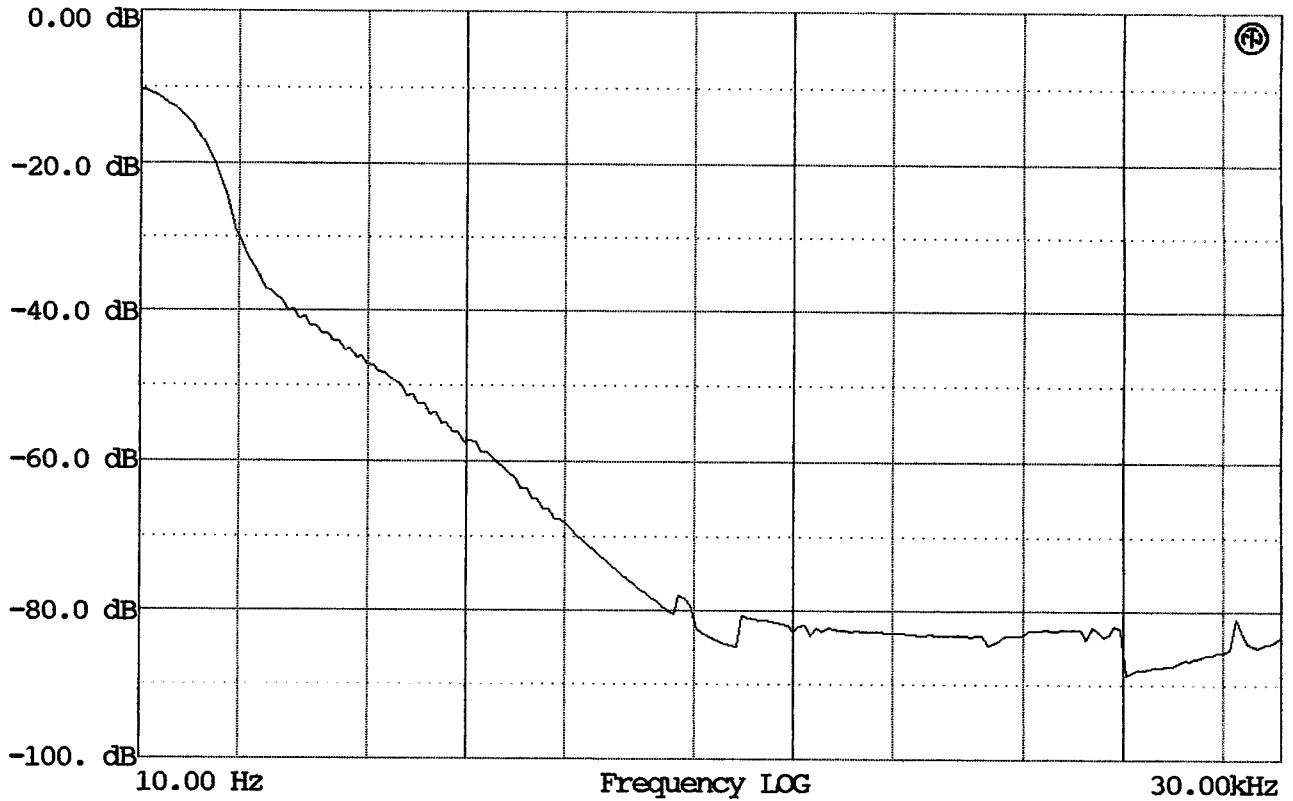


LEVEL
02.07.2011
15:01:41

Output: Analog
Imp: 600Ohm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm
A: -4.36dBV 39.99 Hz

Filter:
Off

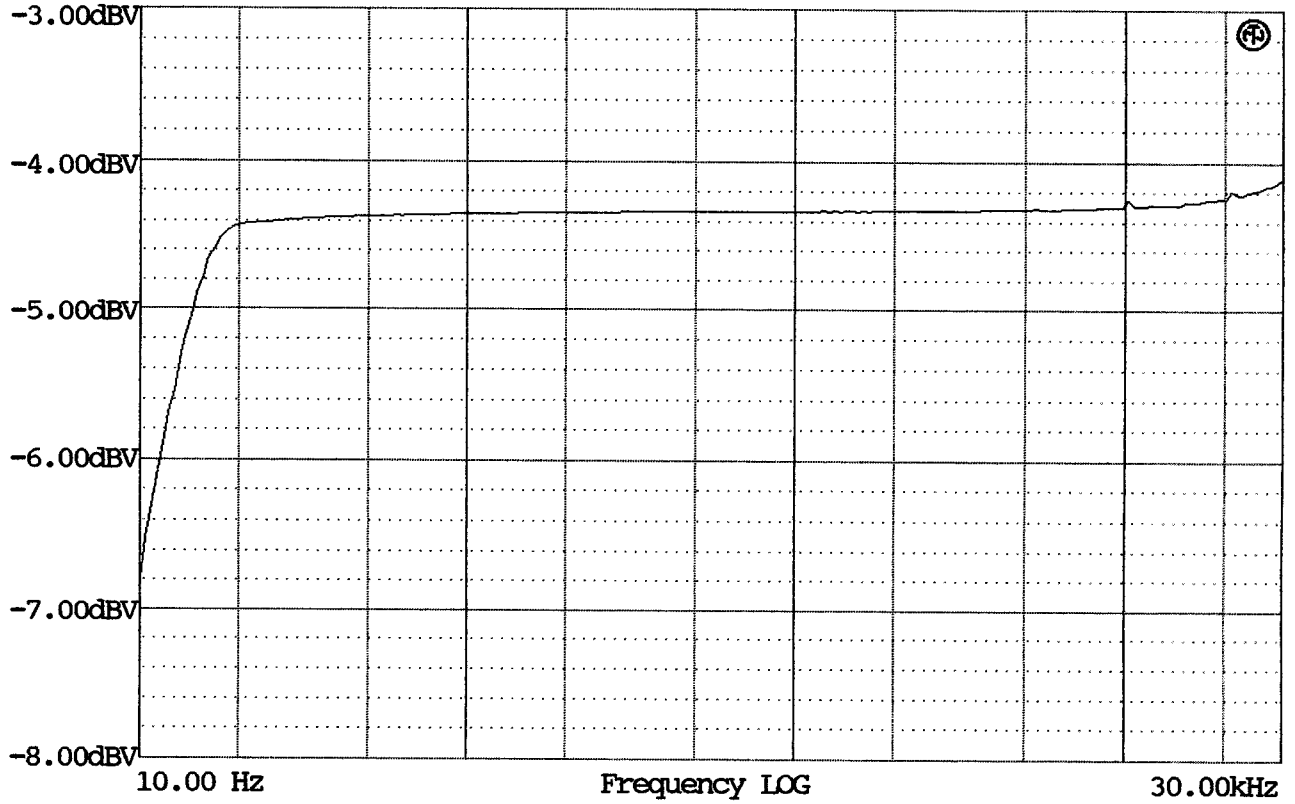


THD+N
02.07.2011
15:23:28

Output: Analog
Imp: 600Ohm
Sine
10.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm
A: -4.35dBV 39.99 Hz

Filter:
Off

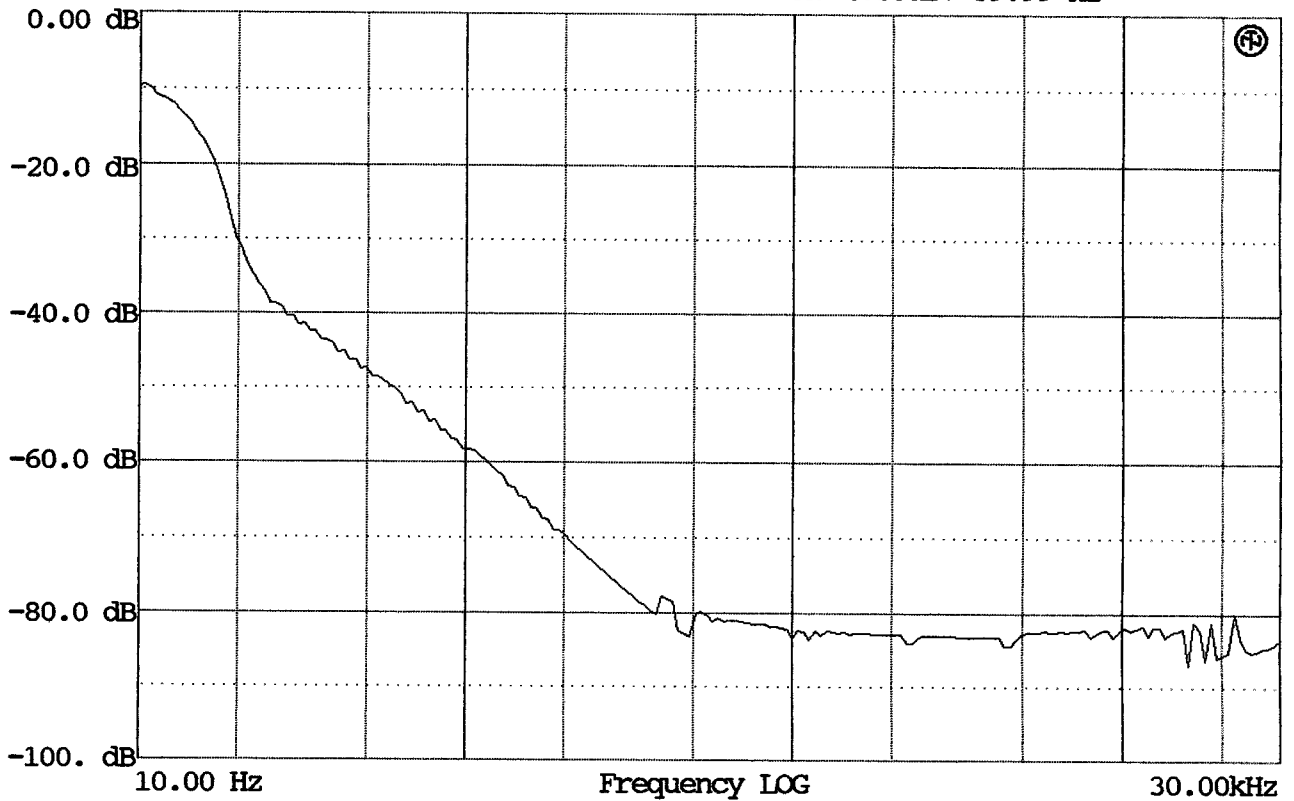


LEVEL
02.07.2011
15:32:51

Output: Analog
Imp: <150hm
Sine
20.0dBV 40.00 Hz

Input: Analog
Imp:100kOhm

Filter:
Off

A: 5.74dBV 39.99 Hz

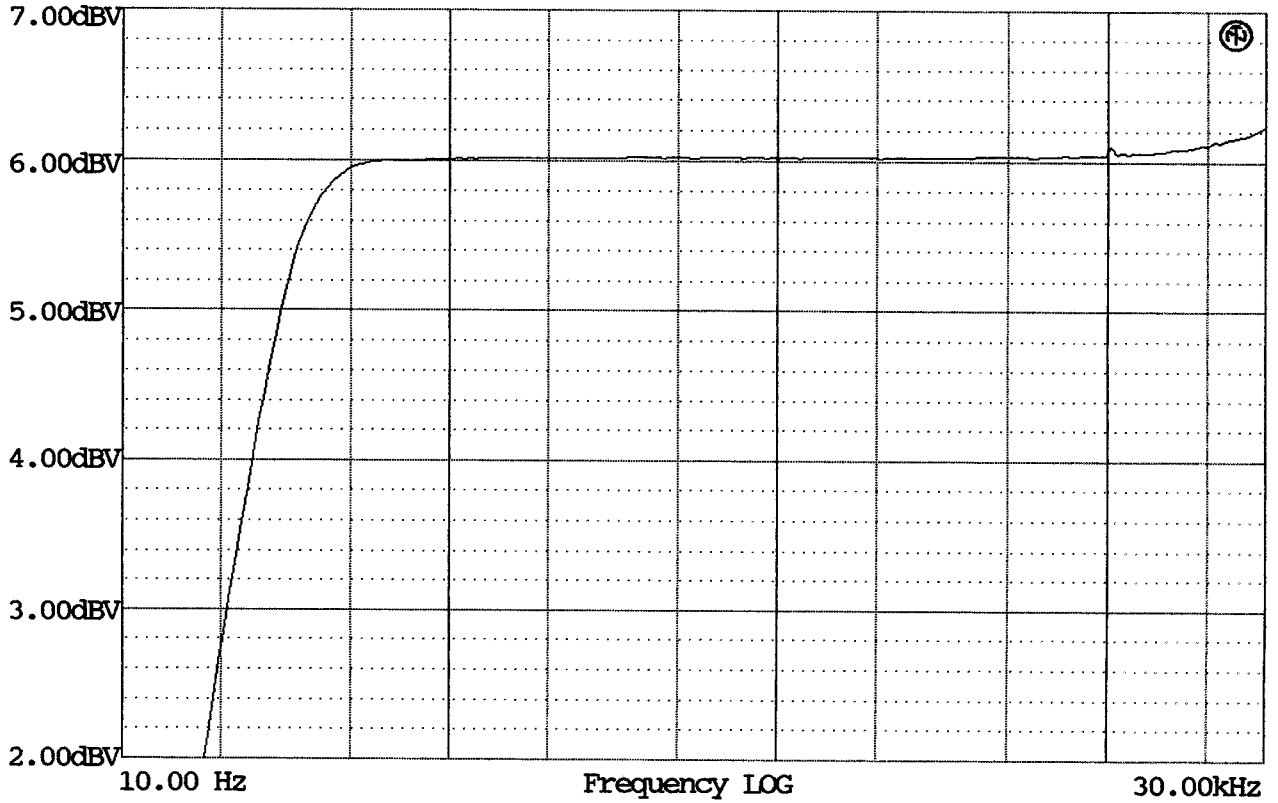


THD+N
02.07.2011
15:50:39

Output: Analog
Imp: <150hm
Sine
20.0dBV 40.00 Hz

Input: Analog
Imp:100kOhm

Filter:
Off

A: 5.74dBV 39.99 Hz

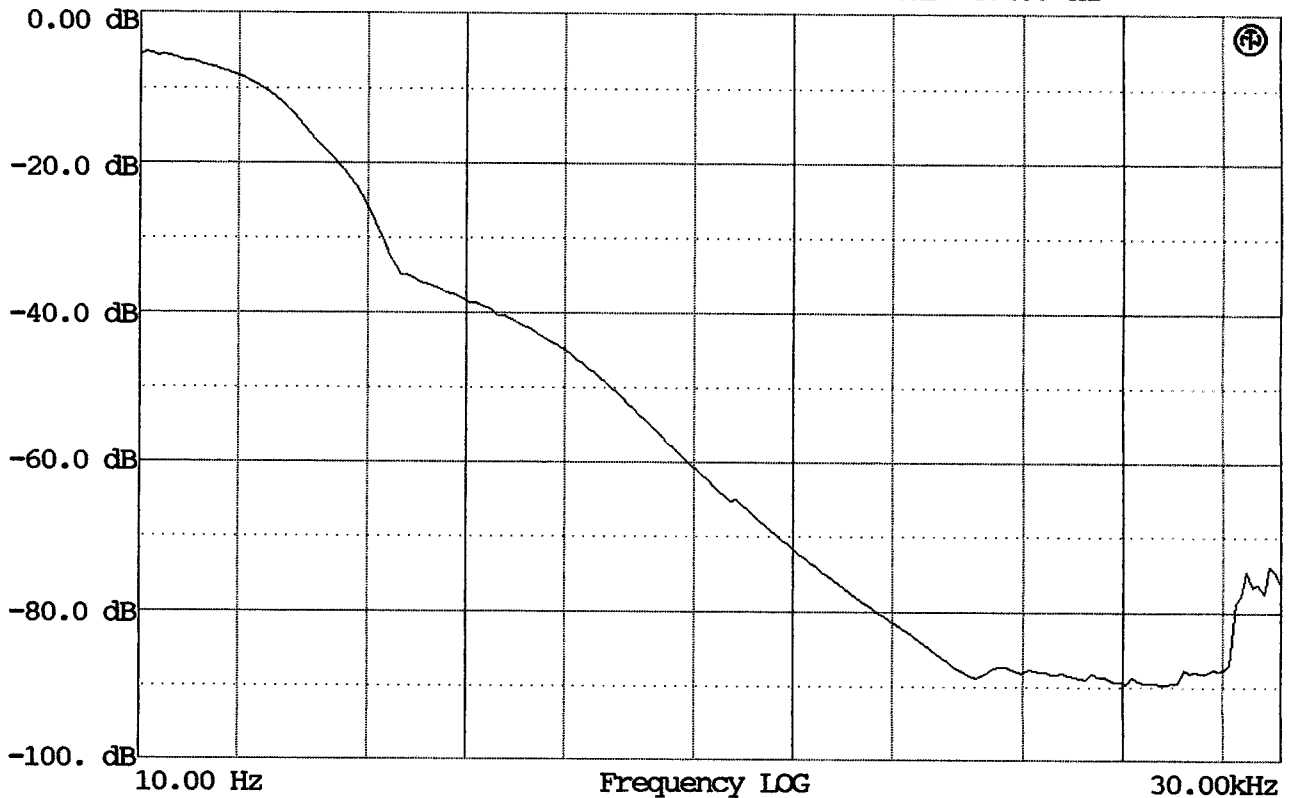


LEVEL
02.07.2011
15:25:44

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 5.32dBV 39.99 Hz

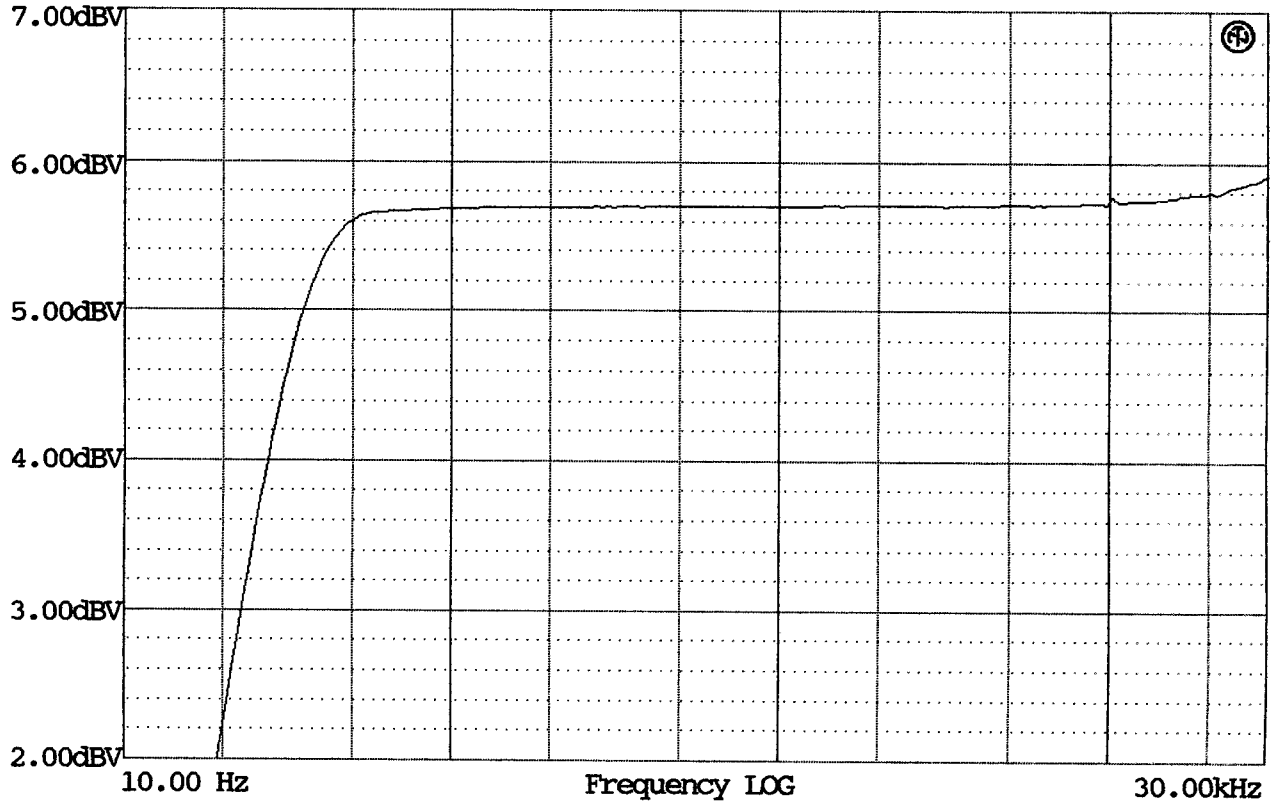

THD+N
02.07.2011
15:31:07

Output: Analog
Imp: 600Ohm
Sine
20.0dBV 40.00 Hz

Input: Analog
Imp: 100kOhm

Filter:
Off

A: 5.32dBV 39.99 Hz

